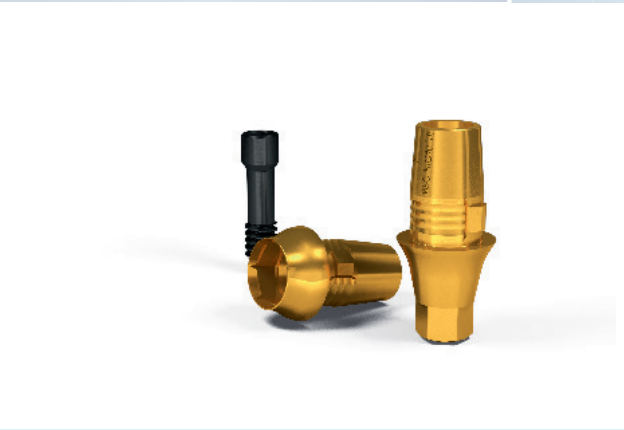
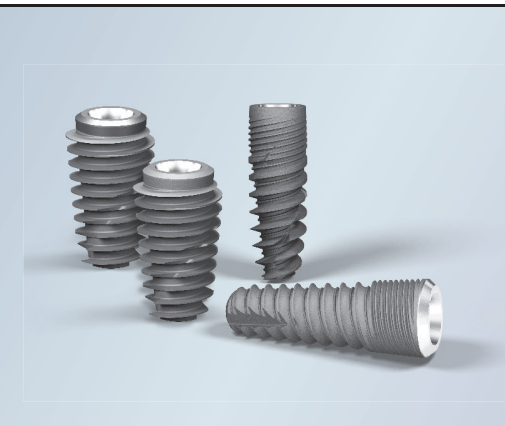



BONE LEVEL AND BONE LEVEL Ø3

i bone® Naturactis Naturall+ Naturactis Ø3 Naturall+ Ø3



IPHYSIO® - PROFILE DESIGNER


FOR BONE LEVEL DENTAL IMPLANTS



IPHYSIO®



IPHYSIO® SHORT



ANGULATED IPHYSIO®

- Delivered with a fixing screw

 Medical grade titanium.

 15 N.cm

	SHAPES			
	A	B	C	D
H 1	NCI_I.A1	NCI_I.B1	NCI_I.C1	NCI_I.D1
H 2	NCI_I.A2	NCI_I.B2	NCI_I.C2	NCI_I.D2
H 4	NCI_I.A4	NCI_I.B4	NCI_I.C4	NCI_I.D4

	SHAPES	
	B	C
H 2 SHORT	NCI_I.B2S	NCI_I.C2S
H 3 SHORT	NCI_I.B3S	NCI_I.C3S

	SHAPES A2
10°	NCI_I.A2.10
20°	NCI_I.A2.20

BONE PROFILERS



guide screw
Ref. NVD_35

SHAPES B	SHAPES C
NTD35	NFE_60.52P

IPHYSIO® TRY IN ABUTMENT KIT



 This kit contains 16 trial abutments (2 angulated / 4 shapes / 5 heights) in titanium.

REFERENCE KIE_3N

IPHYSIO® TEMPORARY ABUTMENT



 Clip on temporary abutment - Delivered with the screw
NVP_E35LAB
REFERENCE NCI_IPPC

TRY IN ABUTMENT - Sold individually



	SHAPES			
	A	B	C	D
H 1	NCI_IE.A1	NCI_IE.B1	NCI_IE.C1	NCI_IE.D1
H 2	NCI_IE.A2	NCI_IE.B2	NCI_IE.C2	NCI_IE.D2
H 3		NCI_IE.B2S	NCI_IE.C2S	
H 4		NCI_IE.B3S	NCI_IE.C3S	
H 4	NCI_IE.A4	NCI_IE.B4	NCI_IE.C4	NCI_IE.D4

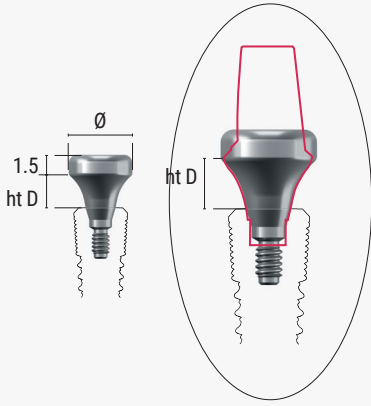
ANGULATED TRY IN ABUTMENT Sold individually



	SHAPES A2
10°	NCI_IE.A2.10
20°	NCI_IE.A2.20

HEALING ABUTMENTS AND COVER SCREWS











HEALING ABUTMENTS

 Healing abutment and final abutment height correspondence	PROSTHETIC PROFILES	HEALING ABUTMENTS REFERENCES	SUPRA-IMPLANT HEIGHTS D
		NCL_36.23	0.5
		NCL_36.34	1.5
		NCL_36.45	2.5
		NCL_36.56	3.5
		NCL_36.67	4.5
		NCL_46.23	0.5
		NCL_46.34	1.5
		NCL_46.45	2.5
		NCL_46.56	3.5
		NCL_46.67	4.5
		NCL_52.23	0.5
		NCL_52.34	1.5
		NCL_52.45	2.5
		NCL_52.56	3.5
		NCL_52.67	4.5
		NCL_60.34*	1.5
		NCL_60.45	2.5
		NCL_60.56	3.5
		NCL_60.67	4.5








COVER SCREW

	 Titane.  Delivered with the implant.  10 N.cm	REFERENCE NVC_35.01
---	---	---------------------

CEMENTED PROSTHESIS ON STRAIGHT AND ANGULATED ABUTMENTS



		EP - Ø 3.6	NP - Ø 4.6	RP - Ø 5.2	WP - Ø 6
TEMPORIZATION					
DIRECT TEMPORARY ABUTMENT (SCREWED) 25 N.CM SUPPLIED WITH A ROTATIONAL CAP: APS_CP36.40 AND NON-ROTATIONAL: APS_CO36.40				NPS_PPT36.40	
TEMPORARY TRANS-SCREWED ABUTMENTS + SCREW: NVP_35LAB 25 N.CM	ROTATIONAL			NPS_PPTR38.2	
	NON-ROTATIONAL			NPS_PPT38.2	
IMPRESSION					
POP-UP IMPRESSION COPING SUPPLIED WITH AN IMPRESSION CAP FOR PICK-UP TECHNIQUE: APS TCP 36 40 + SCREW: NPS VTB 16 174 5 N.CM				NPU_35	
NARROW POP-IN IMPRESSION COPING + SCREW: NPS VTB 16 156 5 N.CM				NPL_37	
LARGE POP-IN IMPRESSION COPING + SCREW : NPS_VTB16.156 5 N.CM				NPL_35	
PICK-UP IMPRESSION COPINGS + SCREW: NPS VG 16 200 (FOR SHORT VERSION) OR NPS VG 16 250 (FOR LONG VERSION) 5 N.CM	SHORT			NPE_T35	
	LONG			NPE_T35L	
IMPLANT ANALOG				ANA_007U	
SCANBODY DIRECT IMPLANT + VIS : NPS_VG16.156 5 N.CM				ETK_NA.35.SB	
LABORATORY SCREW	SHORT			NPS_VG16.156	
				NVP_35LAB	
				NVP_E35LAB	
	MEDIUM			NPS_VG16.200	
	LONG			NPS_VG16.250	

NEXT - CEMENTED PROSTHESIS ON STRAIGHT AND ANGULATED ABUTMENTS

			EP - Ø 3.6	NP - Ø 4.6	RP - Ø 5.2	WP - Ø 6
FINAL RESTORATION						
STRAIGHT ABUTMENTS + SCREW: NVP 35 25 N.CM	H 0.5		NPS_PD36.06	NPS_PD46.06	NPS_PD52.06	-
	H 1.5		NPS_PD36.16	NPS_PD46.16	NPS_PD52.16	NPS_PD60.16*
	H 2.5		NPS_PD36.26	NPS_PD46.26	NPS_PD52.26	NPS_PD60.26
	H 3.5		NPS_PD36.36	NPS_PD46.36	NPS_PD52.36	NPS_PD60.36
	H 4.5		NPS_PD36.46	NPS_PD46.46	NPS_PD52.46	NPS_PD60.46
7° ANGULATED ABUTMENTS + SCREW: NVP 35 25 N.CM	H 0.5		-	NPS_PA46.07.1	NPS_PA52.07.1	-
	H 1.5		NPS_PA36.07.2	NPS_PA46.07.2	NPS_PA52.07.2	NPS_PA60.07.2
	H 2.5		NPS_PA36.07.3	NPS_PA46.07.3	NPS_PA52.07.3	NPS_PA60.07.3
	H 3.5		NPS_PA36.07.4	NPS_PA46.07.4	NPS_PA52.07.4	NPS_PA60.07.4
15° ANGULATED ABUTMENTS + SCREW: NVP 35 25 N.CM	H 0.5		-	NPS_PA46.15.1	NPS_PA52.15.1	-
	H 1.5		NPS_PA36.15.2	NPS_PA46.15.2	NPS_PA52.15.2	NPS_PA60.15.2
	H 2.5		NPS_PA36.15.3	NPS_PA46.15.3	NPS_PA52.15.3	NPS_PA60.15.3
	H 3.5		NPS_PA36.15.4	NPS_PA46.15.4	NPS_PA52.15.4	NPS_PA60.15.4
20° ANGULATED ABUTMENTS + SCREW: NVP 35 25 N.CM	H 0.5		-	NPS_PA46.20.1	NPS_PA52.20.1	-
	H 1.5		NPS_PA36.20.2	NPS_PA46.20.2	NPS_PA52.20.2	NPS_PA60.20.2
	H 2.5		NPS_PA36.20.3	NPS_PA46.20.3	NPS_PA52.20.3	NPS_PA60.20.3
	H 3.5		NPS_PA36.20.4	NPS_PA46.20.4	NPS_PA52.20.4	NPS_PA60.20.4
CASTABLE ABUTMENT COBALT-CHROME BASE + SCREW: NVP E35 25 N.CM	H 0.5		NPS_PCC46.06			
NON-ROTATIONAL ESTHETIBASE INTERFACES + SCREW: NVP E35 25 N.CM	H 1		NPC_PTO40.06			
	H 2		NPC_PTO40.16			
	H 3		NPC_PTO40.26			
	H 4		NPC_PTO40.36			
NON-ROTATIONAL ESTHETIBASE INTERFACES (COMPATIBLE CEREC) + SCREW: NVP_E35 25 N.CM	H 1		NPC_PTO.L			
ROTATIONAL ESTHETIBASE INTERFACES + SCREW: NVP E35 25 N.CM	H 1		NPC_PTC40.06			
	H 2		NPC_PTC40.16			
	H 3		NPC_PTC40.26			
	H 4		NPC_PTC40.36			
ANGULATED ESTHETIBASE BY 10° + VIS : NVP_PTOA35 25 N.CM	H 1		NPC_PTOA40.06.10			To screw on angulated esthetibase, use : - Ball Screwdriver ref.CCR_HE14.X or - Ball mandrel ref.CMR_HE14.L
	H 2		NPC_PTOA40.16.10			
ANGULATED ESTHETIBASE BY 20° + VIS : NVP_PTOA35 25 N.CM	H 1		NPC_PTOA40.06.20			
	H 2		NPC_PTOA40.16.20			

H = SUPRA-IMPLANT HEIGHT * DO NOT USE WITH Naturactis

CEMENTED PROSTHESIS ON DIRECT CLIP ABUTMENTS

			Ø 3.6		Ø 4.8	
			HT 4	HT 5.5	HT 4	HT 5.5
FINAL ABUTMENT SEATING						
DIRECT CLIP ABUTMENTS 35 N.CM	H 0.5		NPS_PP 36.40.1	NPS_PP36.55.1	NPS_PP48.40.1	NPS_PP48.55.1
	H 1.5		NPS_PP36.40.2	NPS_PP36.55.2	NPS_PP48.40.2	NPS_PP48.55.2
	H 2.5		NPS_PP36.40.3	NPS_PP36.55.3	NPS_PP48.40.3	NPS_PP48.55.3
	H 3.5		NPS_PP36.40.4	NPS_PP36.55.4	NPS_PP48.40.4	NPS_PP48.55.4
	H 4.5		NPS_PP36.40.5	NPS_PP36.55.5	NPS_PP48.40.5	NPS_PP48.55.5
TEMPORIZATION						
PROTECTION CAPS			APS_CP36.40	APS_CP36.55	APS_CP48.40	APS_CP48.55
IMPRESSION						
CLIP-ON TRANSFER			APS_TCP36.40	APS_TCP36.55	APS_TCP48.40	APS_TCP48.55
CLIP-ON OPEN IMPRESSION COPINGS FOR ADJUSTED ABUTMENTS			APS_TCP36		APS_TCP48	
DIRECT CLIP ABUTMENT ANALOGS			APS_H36.40	APS_H36.55	APS_H48.40	APS_H48.55
FINAL RESTORATION						
BURN-OUT	ROTATIONAL	H 7		-	-	
		H 10		APS_BCC36.100	APS_BCC48.100	
	NON-ROTATIONAL	H 7		-	-	
		H 10		APS_BCO36.100	APS_BCO48.100	





H = SUPRA-IMPLANT HEIGHT

SCREWED PROSTHESIS ON TETRA CONICAL ABUTMENTS






FINAL ABUTMENT SEATING				
TETRA STRAIGHT ABUTMENTS 35 N.CM	For screwing, use the Internal hex screwdriver Ref.CCL_HI20.24 or the internal hex mandrel Ref.UMA_HI20.26	H 0.5		NPV_PT48.1
		H 1.5		NPV_PT48.2
		H 2.5		NPV_PT48.3
		H 3.5		NPV_PT48.4
		H 4.5		NPV_PT48.5
17° TETRA ANGULATED ABUTMENTS + SCREW: NVP E35 25 N.CM		H 2.5		NPV_PTA48.17.25
		H 3.5		NPV_PTA48.17.35
		H 4.5		NPV_PTA48.17.45
30° TETRA ANGULATED ABUTMENTS + SCREW: NVP E35 25 N.CM		H 3.5		NPV_PTA48.30.35
		H 4.5		NPV_PTA48.30.45
		H 5.5		NPV_PTA48.30.55
TEMPORIZATION				
PROTECTION CAPS 10 N.CM	SHORT			UPV_CPT48.20
	LONG			UPV_CPT48.40
TEMPORARY ABUTMENTS + SCREW: UPV VMD 14 38 20 N.CM	ROTATIONAL			UPV_PMT48.110
	NON-ROTATIONAL			UPV_POT48.110
IMPRESSION				
PICK-UP IMPRESSION COPINGS + SCREW: UPV VGM 14 150 5 N.CM	ROTATIONAL			UPV_TM48
	NON-ROTATIONAL			UPV_TO48
POP-IN IMPRESSION COPING 5 N.CM (SHORT SCANBODY)	ROTATIONAL			UPV_PI48
TETRA ABUTMENTS ANALOG				UPV_HM48
TETRA ABUTMENTS DIGITAL ANALOG				ANA_039U
LABORATORY SCREW	SHORT			UPV_VGM14.40
	MEDIUM			UPV_VGM14.150
	LONG			UPV_VGM14.200
SCANBODY ON TETRA ABUTMENTS + SCREW: NPV VG 14 105 5 N.CM	ROTATIONAL			ETK_UN.SBP
	NON-ROTATIONAL			ETK_UN.SBPO
FINAL RESTORATION				
BURN-OUT + SCREW: UPV VMD 14 38 20 N.CM	ROTATIONAL			UPV_CMC48.110
CASTABLE ABUTMENT WITH CHROME COBALT BASE + SCREW: UPV VMD 14 38 - 20 N.CM	NON-ROTATIONAL			UPV_PCC48.110
ESTHETIBASE INTERFACE ON TETRA ABUTMENT + SCREW UPV_VMD14.38 - 20 N.CM	H 1.3			UPV_PTC

H = SUPRA-IMPLANT HEIGHT

BRIDGE ON ABUTMENTS WITH FINS ALL IN BAR®



WINGED COPINGS			
CENTERED ABUTMENT SUPPLIED WITH A FIXING SCREW (REF. UPV VMD 14 38) TITANIUM 20 N.CM	SHORT		ARS_PT_AC
	LONG		ARS_PT_AC.30
OFF-CENTER ABUTMENT SUPPLIED WITH A FIXING SCREW (REF. UPV VMD 14 38) TITANIUM 20 N.CM	SHORT		ARS_PT_AT
	LONG		ARS_PT_AT.30

SCREWED PROSTHESIS ON PLURAL STRAIGHT CONICAL ABUTMENTS

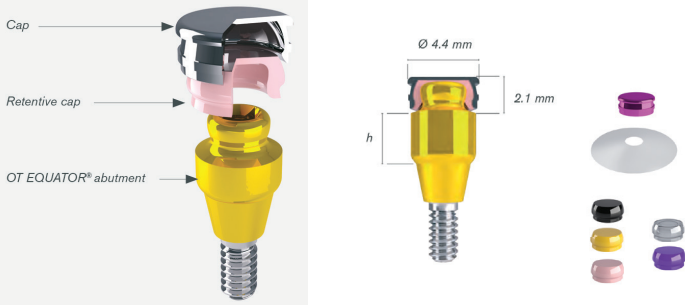
FINAL ABUTMENT SEATING			
STRAIGHT PLURAL ABUTMENTS 35 N.CM	H 0.5		NPV_PP31.07
	H 1.5		NPV_PP31.18
	H 2.5		NPV_PP31.28
	H 3.5		NPV_PP31.38
	H 4.5		NPV_PP31.48
TEMPORIZATION			
TEMPORARY CAP 10 N.CM			NPV_CPP38.32
TEMPORARY ABUTMENT + SCREW: NPV VP 18 56 20 N.CM			NPV_PPT46.100
IMPRESSION			
PICK-UP IMPRESSION COPING + SCREW: NPV VG 18 105 5 N.CM			NPV_TP4X
PLURAL STRAIGHT ABUTMENT ANALOG			ANA_026U
LABORATORY SCREW			NPV_VG18.105
SCANBODY ON PLURAL STRAIGHT ABUTMENT + SCREW: NPV VP 18 56 5 N.CM			ETK_NA.SPD
FINAL RESTORATION			
BURN-OUT + SCREW: NPV VP 18 56 20 N.CM	Ø 4.6		NPV_CCP35.46

H = SUPRA-IMPLANT HEIGHT

REMOVABLE PROSTHESIS ON O-RING ABUTMENTS

FINAL ABUTMENT SEATING			
O'RING ABUTMENT 35 N.CM	H 1.5		NPA_OR35.29.MALE
	H 3.5		NPA_OR35.40.MALE
	H 5.5		NPA_OR35.60.MALE
IMPRESSION			
IMPRESSION ON O'RING ABUTMENT			
ANALOG			OPS_HOBI
FINAL RESTORATION			
O'RING DELIVERED WITH 60 SHORES SEAL			UPA_FOR52
O'RING SEALS	50 SHORES		UPA_JOR50
	60 SHORES		UPA_JOR60
	70 SHORES		UPA_JOR70
O'RING INTERNAL HEX MANDREL			CMO_HI.2526


REMOVABLE PROSTHESIS ON EQUATOR® ABUTMENTS

FINAL ABUTMENT SEATING			
KIT OT EQUATOR® 25 N.CM	H 1		130 NAT 1
	H 2		130 NAT 2
	H 3		130 NAT 3
	H 4		130 NAT 4
	H 5		130NAT05
	H 6		130NAT06
	H 7		130NAT07
IMPRESSION COPING PACK OF 2			044 CAIN
ANALOG EQUATOR® PACK OF 2			144 AE
FINAL RESTORATION			
SHEATH KIT			192 ECE
SMART BOX KIT			335 SBC
EQUATOR® MANDREL SCREWDRIVER			760CE
INSERTION TOOL AND SHEATH EXTRACTION			485IC

IPHYSIO® - PROFILE DESIGNER

FOR BONE LEVEL Ø3 DENTAL IMPLANTS

IPHYSIO® - *Delivered with a fixing screw*



 Medical grade titanium.

 15 N.cm

	SHAPE
	A
H 2	NCl3_I.A2
H 4	NCl3_I.A4

IPHYSIO® TEMPORARY ABUTMENTS

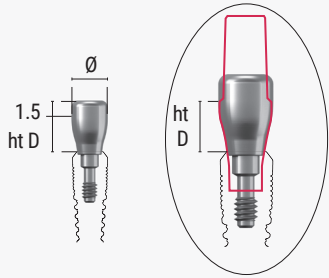


 Clip on temporary abutment - Delivered with the screw NVP_33

REFERENCE NCl3_IPPC

HEALING ABUTMENTS AND COVER SCREWS

HEALING ABUTMENTS



Healing abutment and final abutment height correspondence

 Titane.

 10 N.cm

PROSTHETIC PROFILES	HEALING ABUTMENTS REFERENCES	SUPRA-IMPLANT HEIGHTS D
	NCl_30.23	0.5
	NCl_30.45	2.5
	NCl_30.67	4.5

COVER SCREW









 Titane.

 Delivered with the implant.

 10 N.cm





REFERENCE NVC_31

CEMENTED PROSTHESIS ON STRAIGHT AND ANGULATED ABUTMENTS

		MP - Ø 3	
TEMPORIZATION			
NON-ROTATIONAL TEMPORARY ABUTMENT + SCREW: NVP 31 20 N.CM			NPS_PPT30.1
IMPRESSION			
POP-IN IMPRESSION COPING + SCREW: NPS VTB 14 156 5 N.CM			NPI_31
PICK-UP IMPRESSION COPING + SCREW: NPS VG 14 200 5 N.CM			NPE_T30
ANALOG			ANA_004U
SCANBODY DIRECT ON IMPLANT + SCREW: NVP 31 5 N.CM			ETK_NA30.SB
LABORATORY GUIDE SCREWS 5 N.CM	MEDIUM		NPS_VG14.200
	LONG		NPS_VG14.250
FINAL RESTORATION			
STRAIGHT ABUTMENTS + SCREW: NVP 31 20 N.CM	H 1		NPS_PD30.06
	H 3		NPS_PD30.26
	H 5		NPS_PD30.46
7° ANGULATED ABUTMENTS + SCREW: NVP 31 20 N.CM	H 1		NPS_PA30.07.1
	H 3		NPS_PA30.07.3
15° ANGULATED ABUTMENTS + SCREW: NVP 31 20 N.CM	H 1		NPS_PA30.15.1
	H 3		NPS_PA30.15.3
CASTABLE ABUTMENT COBALT-CHROME BASE + SCREW: NVP 31 20 N.CM			NPS_PCC30.16
NON-ROTATIONAL ESTHETIBASE INTERFACES + SCREW: NVP 31 20 N.CM	H 2		NPC_PT030.16
	H 3		NPC_PT030.26



H = SUPRA-IMPLANT HEIGHT

CEMENTED PROSTHESIS ON DIRECT CLIP ABUTMENTS



			EP - Ø 3.6
FINAL ABUTMENT SEATING			
DIRECT CLIP ABUTMENTS 30 N.CM	H 3		NPS_PP30.55.3
TEMPORIZATION			
PROTECTION CAP			APS_CP36.55
IMPRESSION			
CLIP-ON IMPRESSION COPING			APS_TCP36.55
CLIP-ON OPEN IMPRESSION COPING FOR ADJUSTED ABUTMENTS			APS_TCP36
DIRECT CLIP ABUTMENT ANALOG			APS_H36.55
FINAL RESTORATION			
BURN-OUT	ROTATIONAL		APS_BCC36.100
	NON-ROTATIONAL		APS_BC036.100

H = SUPRA-IMPLANT HEIGHT

REMOVABLE PROSTHESIS ON O-RING ABUTMENTS

FINAL ABUTMENT SEATING		
O'RING ABUTMENT 30 N.CM		NPA_OR31.29MALE
IMPRESSION		
IMPRESSION ON O'RING ABUTMENT		
O'RING ANALOG		OPS_HOBI
FINAL RESTORATION		
O'RING DELIVERED WITH 60 SHORES SEAL		UPA_FOR52
O'RING SEALS	50 SHORES	UPA_JOR50
	60 SHORES	UPA_JOR60
	70 SHORES	UPA_JOR70
O'RING INTERNAL HEX MANDREL		CMO_HI.2526

REMOVABLE PROSTHESIS ON EQUATOR® ABUTMENTS

FINAL ABUTMENT SEATING		
KIT OT EQUATOR® Ø3 25 N.CM	H 1 	130NTR1
	H 3 	130NTR3
	H 5 	130NTR5
TRANSFER PACK OF 2		044 CAIN
EQUATOR® ABUTMENT ANALOG PACK OF 2		144 AE
FINAL RESTORATION		
SHEATH KIT		192 ECE
KIT SMART BOX		335 SBC
EQUATOR® SCREWDRIVER CHUCK		760CE
TOOL FOR INSERTING AND EXTRACTION TOOL		485IC



LYRA ETK - 726 rue du Général de Gaulle - 74700 Sallanches - France

Service clients France : T. +33 (0)1 76 42 00 60 | International Customer Service: T. +33 (0)1 76 36 14 04
sales@lyraetk.com | www.lyraetk.com



EUROTEKNIKA S.A.S - 726 rue du Général de Gaulle, 74700 Sallanches (France)

Class I, IIa and IIb medical devices in compliance with European Regulation MDR (EU) 2017/745 (class I) and European Directive 93/42/EEC (classes IIa and IIb) and CE marking (class I) and CE 0459 (class IIa and IIb). Devices not reimbursed by National Insurance, they must be used by oral health professionals. Please read the instructions and user manual carefully.



RHEIN 83 S.R.L - Via Zago 10/ABC 40128 BOLOGNA (BO) (Italy)

EUROTEKNIKA S.A.S - 726 rue du Général de Gaulle, 74700 Sallanches (France)

Class I, IIa and IIb medical devices in compliance with European Regulation MDR (EU) 2017/745 (class I) and European Directive 93/42/EEC (classes IIa and IIb) and CE marking (class I) and CE 0425 (class IIa and IIb). Devices not reimbursed by National Insurance, they must be used by oral health professionals. Please read the instructions and user manual carefully.